


4 Channel Lab Scope

Back Setup Data Cursors Refresh File Print

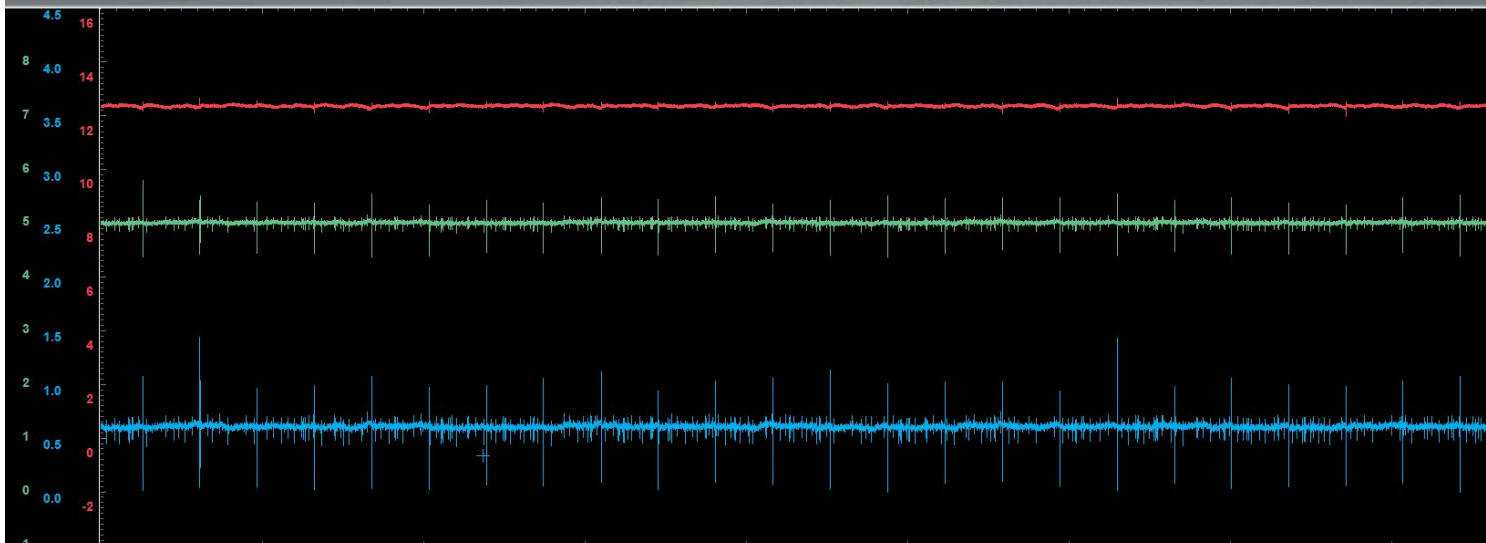

Profile	Channel	Probe	Peak Detect	Filter	Inverted	Coupling AC	Scale
	2						10 V
	3						5 V
	4						20 V
							1 ms

00:01:047